

Pure-AMC

Fluoroscopy-use during ureterorenoscopy: are urologists concerned about radiation exposure? A nationwide survey in Belgium and The Netherlands

Henderickx, Michaël M. E. L.; Baard, Joyce; Beerlage, Harrie P.; Kamphuis, Guido M.

Published in:
Acta chirurgica Belgica

DOI:
[10.1080/00015458.2019.1693150](https://doi.org/10.1080/00015458.2019.1693150)

Published: 01/01/2021

Document Version
Peer reviewed version

Citation for published version (APA):
Henderickx, M. M. E. L., Baard, J., Beerlage, H. P., & Kamphuis, G. M. (2021). Fluoroscopy-use during ureterorenoscopy: are urologists concerned about radiation exposure? A nationwide survey in Belgium and The Netherlands. *Acta chirurgica Belgica*, 121(3), 170-177. <https://doi.org/10.1080/00015458.2019.1693150>

General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal ?

Take down policy

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.



Fluoroscopy-use during ureterorenoscopy: are urologists concerned about radiation exposure? A nationwide survey in Belgium and The Netherlands

Michaël M. E. L. Henderickx, Joyce Baard, Harrie P. Beerlage & Guido M. Kamphuis


To cite this article: Michaël M. E. L. Henderickx, Joyce Baard, Harrie P. Beerlage & Guido M. Kamphuis (2019): Fluoroscopy-use during ureterorenoscopy: are urologists concerned about radiation exposure? A nationwide survey in Belgium and The Netherlands, Acta Chirurgica Belgica, DOI: [10.1080/00015458.2019.1693150](https://doi.org/10.1080/00015458.2019.1693150)

To link to this article: <https://doi.org/10.1080/00015458.2019.1693150>




Accepted author version posted online: 13 Nov 2019.
Published online: 21 Nov 2019.



[Submit your article to this journal](#) 



[View related articles](#) 



[View Crossmark data](#) 

Fluoroscopy-use during ureterorenoscopy: are urologists concerned about radiation exposure? A nationwide survey in Belgium and The Netherlands

Michaël M. E. L. Henderickx , Joyce Baard , Harrie P. Beerlage and Guido M. Kamphuis

Department of Urology, Amsterdam UMC, University of Amsterdam, Amsterdam, The Netherlands

ABSTRACT

Introduction: To evaluate the use and awareness of radiation during URS among Belgian and Dutch urologists.

Material and methods: An online questionnaire was sent to all members of the Belgian and Dutch Association of Urology.

Results: 170 urologists finished the complete questionnaire. 10% of the respondents are not familiar with the ALARA-principle. 29% starts with a KUB and 48% makes an XRPG at the beginning of the procedure. 85% uses fluoroscopy to place a wire or ureteral access sheath, 18% during stone treatment, 59% to screen for missed stones or calyces, 90% to place a JJ-stent or ureter-catheter and 23% to check for extravasation. 82% do not document radiation data. 51% does not wear a dosimeter during fluoroscopy. Almost all wear a lead apron during fluoroscopy, 47% uses additional thyroid shields and only 4% uses lead glasses. 88% intentionally reduces fluoroscopy time, 75% reduces the exposed area with a diaphragm, 72% brings the radiation source close to the patient and 44% uses pulsed fluoroscopy.

Conclusion: There is a wide variety in the use and awareness of radiation during URS. To further reduce radiation and its negative effect for patients and medical staff, awareness about radiation safety should increase among urologists.

Abbreviations: URS: Ureterorenoscopy; NVU: Dutch Association of Urology; BVU: Belgian Association of Urology

ARTICLE HISTORY

Received 20 July 2019

Accepted 10 November 2019

KEYWORDS

Endourology; ureterorenoscopy; survey; fluoroscopy; ALARA-principle

Introduction

According to the ALARA-principle the radiation exposure should be kept *as low as reasonably achievable* to decrease the risk of negative long-term effects of radiation for patients and medical staff [1]. These negative effects are the result of DNA and tissue damage, which can lead to an increased risk of developing cataract, malignancies, skin reactions, sterility or congenital anomalies [2–6].

Shock wave lithotripsy was the treatment of choice for renal calculi for a long time (1982–early 2000) [7]. However, over the last two decades percutaneous nephrolithotripsy and ureterorenoscopy (URS) gained in popularity [8]. The rise of these minimal invasive techniques lead to simultaneous rise in the use of fluoroscopy in urological operation rooms [8,9].

The aim of this survey was to evaluate the use and awareness of radiation during URS and the knowledge of the ALARA-principle among the members of the Dutch (Nederlandse Vereniging

van Urologie, NVU) and Belgian (Belgische Vereniging voor Urologie, BVU) association of urology.

Materials and methods

In August 2018, a hyperlink to an online questionnaire was sent to all members of the NVU and BVU to assess the use and awareness of fluoroscopy during URS and the knowledge of the ALARA-principle among urologists in Belgium and the Netherlands.

The questionnaire was conducted using the web-based SurveyMonkey® system (Palo Alto, California, United States). The hyperlink to the questionnaire was forwarded through e-mail to all members of the NVU and BVU through their respective national association office, accompanied by a short description of the aim of this questionnaire. The questionnaire remained open for one month. No reminder e-mail was sent.

The questionnaire consisted of 14 questions (Appendix). All questions were multiple choice.

For six questions, respondents had the possibility to give a free text response. For three questions, multiple answers were allowed. The questions were divided into three main categories: respondents characteristics (four questions), awareness of the ALARA-principle (five questions) and the use of fluoroscopy during URS (five questions).

Results

The online questionnaire was sent to 413 members of the NVU and 193 members of the BVU. 170 urologists (28%) responded and completed the questionnaire.

Respondents characteristics

Of the 170 respondents, 74% ($n=126$) is Dutch and 26% ($n=44$) is Belgian. 81% ($n=138$) works in a non-academic hospital and 19% ($n=32$) in an academic hospital. 20% of the respondents ($n=34$) are residents, 23% ($n=39$) has 0–5 years of experience, 17% ($n=29$) 6–10 years of experience, 23% ($n=39$) 11–20 years of experience and 17% ($n=29$) has more than 20 years of experience (Table 1).

On a monthly basis, 26% of the respondents ($n=45$) performs 0–5 ureterorenoscopies, 47%

($n=80$) performs 6–10 procedures, 22% ($n=37$) performs 11–20 procedures and 5% ($n=8$) performs over 20 procedures.

The ALARA-principle

10% ($n=17$) of the respondents are not familiar with the ALARA-principle and 6% ($n=11$) did not take any additional radiation protection course. Of the 170 respondents, half (51%, $n=87$) do not wear a dosimeter during fluoroscopy and only 26% ($n=43$) always wears a dosimeter (Figure 1).

To lower the exposure to radiation, 88% ($n=149$) intentionally tries to reduce the fluoroscopy time, whereas 75% ($n=127$) actively collimate with a diaphragm to reduce the exposed area and 72% ($n=122$) lowers the distance between the radiation source and the patient. Finally, 44% ($n=74$) uses pulsed fluoroscopy during URS (Figure 2).

The vast majority of respondents (99%, $n=169$) wears a lead apron to protect themselves during fluoroscopy, 47% ($n=80$) uses an additional thyroid shield as protection and only 4% ($n=7$) wears additional lead glasses. 2% of the respondents ($n=3$) uses a lead screen. None of the respondents uses lead gloves during fluoroscopy-use (Figure 2).

Table 1. Characteristics of respondents.

Nationality	
Belgian	26%
Dutch	74%
Hospital	
Academic	19%
Non-academic	81%
Experience	
Resident	20%
0–5 years	23%
6–10 years	17%
11–20 years	23%
>20 years	17%
Number of URS per month	
0–5 procedures	26%
6–10 procedures	47%
11–20 procedures	22%
>20 procedures	5%

Fluoroscopy-use during URS

29% ($n=50$) of the respondents starts by making a kidney, ureter and bladder X-ray before starting the actual procedure and 48% ($n=82$) makes a retrograde ureteropyelogram at the beginning of the procedure as a standard step of the procedure. 85% ($n=145$) uses fluoroscopy to place a guide wire, safety wire or ureteral access sheath. 18% ($n=30$) uses fluoroscopy during stone treatment and 59% ($n=101$) uses fluoroscopy to screen the collecting system for missed stones or calyces.



Figure 1. The ALARA-principle in daily practice (additional radiation protection course, knowledge of the ALARA-principle, use of a dosimeter during fluoroscopy).

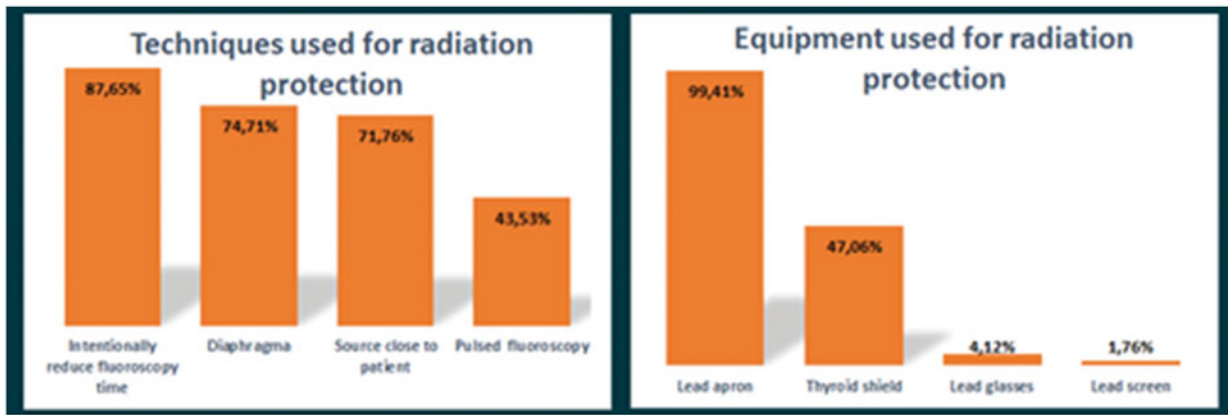


Figure 2. The ALARA-principle in daily practice (techniques used for radiation protection, equipment used for radiation protection).

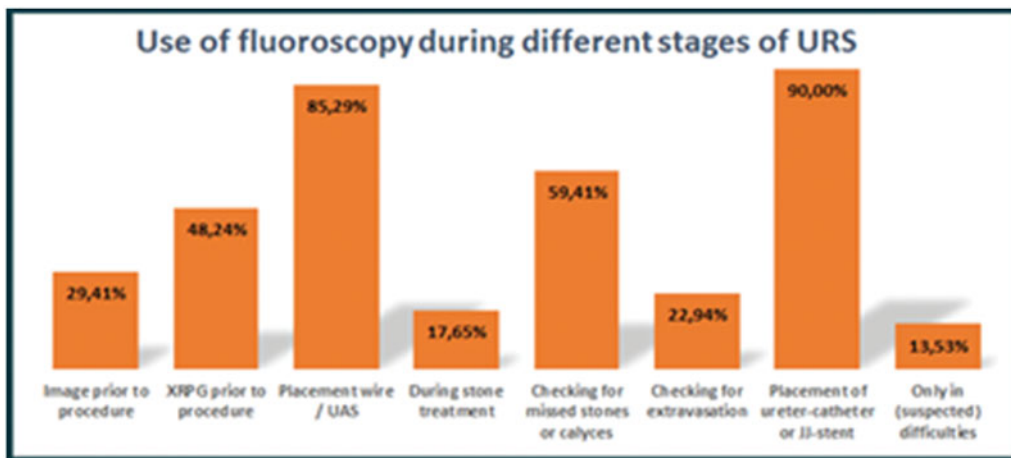


Figure 3. The use of fluoroscopy during different stages of URS.




Figure 4. Fluoroscopy-use during URS (documenting radiation, objectifying stone-free status, operator of fluoroscopy).

23% ($n = 39$) checks for extravasation after the procedure. 90% of respondents ($n = 153$) uses fluoroscopy to place a JJ-stent or ureter-catheter. Finally, 14% ($n = 23$) only uses fluoroscopy when they expect or have difficulties (Figure 3).

22% ($n = 38$) of the respondents operates the fluoroscopy themselves, whereas 78% ($n = 132$) have a radiology technician or OR-nurse who operates the fluoroscopy (Figure 4).

48% ($n = 82$) objectify stone-free status endoscopically, where 50% ($n = 86$) uses endoscopy and fluoroscopy combined to check stone-free status.

82% ($n = 140$) do not document the radiation time or dose after a procedure, whereas 8% ($n = 13$) documents both. 6% ($n = 10$) only documents radiation dose and 4% ($n = 7$) only documents radiation time (Figure 4).

Discussion

The rise of minimally invasive techniques to treat stones has led to a rise in the use of fluoroscopy in modern urological practice [5,9]. Consequently, radiation safety has gained in importance. Patients

and medical staff who receive high cumulative radiation exposure have an increased risk of developing malignancies, skin reactions, cataract, sterility and aplastic anemia [2,4–6].

The risk of developing malignancies increases with an increased exposure to radiation. However, no lower limit is known under which there are no harmful effects. Urologists play a key role in minimizing the radiation exposure for patients and medical staff.⁵ Different studies show that medical doctors are unaware of the radiation levels they are exposed to and even underestimate the actual exposure [10–12].

This reflects in our results, where only 26% always wears a dosimeter, although 94% has followed an additional radiation protection course and 90% is familiar with the ALARA-principle. 20% of our respondents are residents, which explains why this number is not 100%. As it is mandatory for all medical personal in Belgium and the Netherlands, who operate or are actively involved in fluoroscopy, to have additional schooling in radiation protection [13,14].

Our results show that 99% of respondents wear a lead apron to protect themselves during fluoroscopy and 47% uses an additional thyroid shield. Only a minority uses lead glasses (4%), a lead screen (2%) or lead gloves (0%). These results are in line with the data from Friedman et al. [5] They describe an under usage of lead glasses (17–23%), lead gloves (10–33%) and dosimeters (26–34%) and a satisfactory usage of lead aprons (99%) and thyroid shields (24%).

Kim et al. [15] state that the use of a knee-length lead apron and thyroid shield is a minimum in the protection against radiation. The additional use of lead glasses and lead gloves could lower radiation exposure to the eyes and hands respectively with 70–92% and 76.6% [15–17]. In addition, Kim et al. [15] advocate to actively reduce the fluoroscopy time and to use pulsed fluoroscopy. They state that preoperative knowledge of the anatomy can help to reduce the need of per-operative fluoroscopy. Furthermore it is important for urologists to keep distance from the radiation source and to keep their hands out of the radiation beam. Finally they advocate the use of a dosimeter to raise awareness about the received radiation dose.

Horsburgh and Higgins [18] have similar conclusions. They found that sitting during fluoroscopy use increased the dose by 78% compared to standing, as surgeons tend to be closer to the patient when sitting, and therefore advise a

standing position to perform fluoroscopically guided procedures. This study also showed a reduction in radiation dose of 67–77% with pulsed fluoroscopy, 12–47% with collimation with a diaphragm and 5–25% by increasing the distance to the radiation source, however this resulted in an increase in radiation dose for the eyes and thyroid due to scattering. These three techniques also help to lower the radiation dose for the patient.

The major limitation of this survey is the low response rate of 28% with the risk of responders bias. Urology residents and urologists with an affinity for endourology will be more likely to respond, which can lead to sampling and non-response biases [19]. Then again, not all urology residents and urologists perform ureterorenoscopy in Belgium and the Netherlands. Therefore, they should be excluded from the possible responders. Consequently, it can be assumed that the relative response rate (response rate from members performing ureterorenoscopy) is higher than the absolute response rate (response rate from all members), leading to a good overview of the awareness of radiation exposure and knowledge of the ALARA-principle in Belgium and the Netherlands. Furthermore, the response rate for this survey is higher than comparable surveys concerning endourology (14.9%, 20.7%, 23%) sent to a general population of urology residents and/or urologists [20–22].

Another limitation is the lack of evidence of unvalidated survey instruments [19,23]. This makes it hard to predict the reproducibility of this study. Hence, the obtained answers only serve to give a general image and insight on the awareness of radiation exposure and knowledge of the ALARA-principle in Belgium and the Netherlands.

This study wants to emphasize the importance of awareness of radiation exposure for the urologist, the patient and the medical staff. This can be achieved by proper knowledge of the ALARA-principle and the use of a dosimeter during fluoroscopically guided procedures. Furthermore, it is important to reduce the risks of radiation exposure by using personal protection and not to underestimate the risk for the eyes and hands during these procedures. Finally, adequate use and good knowledge of the fluoroscopy will lower radiation exposure.

Conclusion

Fluoroscopy is commonly used during URS by urologists in Belgium and the Netherlands. A majority

is reducing negative radiation effects through additional education, personal protection and the implementation of the ALARA-principle in their daily practice. However, this survey shows a wide variety in the use of radiation during URS, suggesting differences in cumulative radiation dose and thus room to reduce both radiation and the subsequent negative effect for patients and medical staff. Therefore, awareness about radiation safety should increase among urologists.

Acknowledgments

The authors wish to thank all the members of the NVU and BVU who participated in the survey and the offices of NVU and BVU that have assisted with the distribution of the survey.

ORCID

Michaël M. E. L. Henderickx  <http://orcid.org/0000-0002-8277-0046>

Joyce Baard  <http://orcid.org/0000-0002-5509-0213>

Guido M. Kamphuis  <http://orcid.org/0000-0002-4583-4231>

References

- [1] Siegel JA, McCollough CH, Orton CG. Advocating for use of the ALARA principle in the context of medical imaging fails to recognize that the risk is hypothetical and so serves to reinforce patients' fears of radiation. *Med Phys*. 2017;44(1):3–6.
- [2] Linet MS, Slovis TL, Miller DL, et al. Cancer risks associated with external radiation from diagnostic imaging procedures. *Cancer J Clin*. 2012;62(2):75–100.
- [3] Kal HB, Struikmans H. Pregnancy and medical irradiation; summary and conclusion from the international commission on radiological protection, publication 84. *Ned Tijdschrift Geneesk*. 2002;146:299–303.
- [4] Lim HS. Health disorders caused by physical factors among health care workers: focusing on ionizing radiation. *J Korean Med Assoc*. 2010;53(6):483–491.
- [5] Friedman AA, Ghani KR, Peabody JO, et al. Radiation safety knowledge and practices among urology residents and fellows: results of a nationwide survey. *J Surg*. 2013; 70(2):224–231.
- [6] Koenig TR, Wolff D, Mettler FA, et al. Skin injuries from fluoroscopically guided procedures: part 1, characteristics of radiation injury. *AJR AM J Roentgenol*. 2001;177(1):3–11.
- [7] Tunc L, Tokgoz H, Tan MO, Kupeli B, et al. Stones in anomalous kidneys: results of treatment by shock wave lithotripsy in 150 patients. *Int J Urol*. 2004; 11(10):831–836.
- [8] Galonnier F, Traxer O, Rosec M, et al. Surgical staff radiation protection during fluoroscopy-guided urological interventions. *J Endourol*. 2016;30(6):638–643.
- [9] Bratslavsky G, Moran ME. Current trends in ureteroscopy. *Urol Clin North Am*. 2004;31(1):181–187.
- [10] Bosanquet DC, Green G, Bosanquet AJ, et al. Doctor's knowledge of radiation – a two-centre study and historical comparison. *Clin Radiol*. 2011; 66(8):748–751.
- [11] Keijzers GB, Britton CJ. Doctors' knowledge of patient radiation exposure from diagnostic imaging requested in the emergency department. *Med J Aust*. 2010;193(8):450–453.
- [12] Barnawi RA, Alrefai WM, Qari F, et al. Khafaji M: Doctors' knowledge of the doses and risk of radiological investigations performed in the emergency department. *Saudi Med J*. 2018; 39(11):1130–1138.
- [13] FANC federaal agentschap voor nucleaire controle. Blootstelling van patiënten: bijkomende opleiding. <https://fanc.fgov.be/nl/professionelen/medische-professionelen/helpers/blootstelling-van-patienten-bijkomende-opleiding>. Accessed 3 May 2019.
- [14] Staatsblad van het Koninkrijk der Nederlanden. Besluit van 23 oktober 2017, houdende vaststelling van regels ter bescherming van personen tegen gevaren van blootstelling aan ioniserende straling (besluit basisveiligheidsnormen stralingbescherming). <file:///H:/Downloads/Publicatie+Staatsblad+Bbs.pdf>. Accessed 3 May 2019.
- [15] Kim CH, Kim SJ, Kim MH, et al. Are Urologists Performing Semi-rigid Ureteroscopic Lithotripsy Safe From Radiation Exposure? A Guidance to Reduce the Radiation Dose. *Urology*. 2016;95:54–59.
- [16] Agarwal SK, Friesen EJ, Huddleston AL, et al. The effectiveness of glass lenses in reducing exposure to the eyes. *Radiology*. 1978;129(3):810–811.
- [17] Hohl C, Suess C, Wildberger JE, et al. Dose reduction during CT fluoroscopy: phantom study of angular beam modulation. *Radiology*. 2008;246(2): 519–525.
- [18] Horsburgh BA, Higgins M. A study of occupational radiation dosimetry during fluoroscopically guided simulated urological surgery in the lithotomy position. *J Endourol*. 2016;30(12):1312–1320.
- [19] Pereira JF, Bower P, Jung E, et al. Ureteral stenting practices following routine ureteroscopy: an international survey. *World J Urol*. 2019;37(11):2501. [Epub ahead of print]
- [20] Söylemez H, Sancaktutar AA, Silay MS, et al. Knowledge and attitude of European urology residents about ionizing radiation. *Urology*. 2013;81(1): 30–36.
- [21] Dauw CA, Simeon L, Alruwaily AF, et al. Contemporary practice patterns of flexible ureteroscopy for treating renal stones: results of a worldwide survey. *J Endourol*. 2015; 29(11):1221–1230.
- [22] Bandi G, Best SL, Nakada SY. Current practice patterns in the management of upper urinary tract calculi in the north central United States. *J Endourol*. 2008;22(4):631–636.
- [23] Proietti S, Somani BK, Pietropaolo A, et al. Italian endourological panorama: results from a national survey. *Cent European J Urol*. 2018;71(2):190–195.

Appendix

1. In welk land bent U werkzaam?

- België Nederland
- overige (geef nadere toelichting)

2. In welk type ziekenhuis bent U werkzaam?

- perifere ziekenhuis
- academisch ziekenhuis

3. Hoelang bent U reeds werkzaam als uroloog?

- arts-assistent in opleiding 11-20 jaar
- 0-5 jaar >20 jaar
- 6-10 jaar

4. Door wie wordt de stralenbron bestuurd tijdens een URS?

- operateur zelf OK-verpleegkundige / OK-assistent
- radioloog arts-assistent / co-assistent
- radiologie-medewerker
- overige (geef nadere toelichting)

5. Heeft U een aanvullende cursus radioprotectie / stralenbescherming gevolgd?

- neen
- ja, 0-5 jaar geleden
- ja, 5-10 jaar geleden
- ja, >10 jaar geleden

6. Is het ALARA-principe U bekend en houdt U er bewust rekening mee?

- ja, het ALARA-principe is me bekend en ik probeer de stralenbelasting zelf bewust te beperken
- ja, het ALARA-principe is me bekend, maar ik laat het beperken van de stralenbelasting over aan de medewerker die de stralenbron bestuurt
- ja, het ALARA-principe is me bekend, maar ik hou er geen rekening mee
- neen, het ALARA-principe is me niet bekend

7. Welke technieken gebruikt U of Uw medewerker die de stralenbron bestuurt om de stralenbelasting te beperken (meerdere antwoorden zijn mogelijk)?

- | | |
|--|---|
| <input type="checkbox"/> de stralenbron dicht bij de patiënt brengen | <input type="checkbox"/> gepulseerd doorlichten |
| <input type="checkbox"/> de doorlichtingsdosis met opzicht beperken | <input type="checkbox"/> diafragmeren |
| <input type="checkbox"/> de doorlichtingstijd met opzicht beperken | |
| <input type="checkbox"/> overige (geef nadere toelichting) | |

8. Welke van de volgende beschermingsmiddelen gebruikt U tijdens het gebruik van röntgenstralen (meerdere antwoorden zijn mogelijk)?

- | | |
|--|--|
| <input type="checkbox"/> loodschort | <input type="checkbox"/> loden handschoenen |
| <input type="checkbox"/> loodbril | <input type="checkbox"/> loodschermb voor de stralenbron |
| <input type="checkbox"/> loden halskraag | <input type="checkbox"/> geen |
| <input type="checkbox"/> overige (geef nadere toelichting) | |

9. Draagt U bij het gebruik van röntgenstralen een dosimeter?

- ja, altijd
- ja, meestal
- ja, soms
- neen, nooit

10. Wat vindt U van het gebruik van röntgenstralen tijdens een URS?

- | | |
|--|--|
| <input type="radio"/> altijd noodzakelijk | <input type="radio"/> enkel noodzakelijk bij problemen |
| <input type="radio"/> meestal noodzakelijk | <input type="radio"/> overbodig |
| <input type="radio"/> soms noodzakelijk | |

11. Hoeveel URS'en voert U gemiddeld als eerste operateur of supervisor uit per maand?

- 0-5
- 6-10
- 11-20
- >20

=

12. Bij welke stappen van een URS gebruikt U (in de meeste gevallen) röntgenstralen (meerdere antwoorden zijn mogelijk):

- | | |
|--|--|
| <input type="checkbox"/> blanco opname voor aanvang van de URS | <input type="checkbox"/> beoordeling van het systeem om na te gaan dat er geen stenen of kelken gemist zijn |
| <input type="checkbox"/> retrograde ureteropyelografie voor aanvang van de URS | <input type="checkbox"/> beoordeling van het systeem om na te gaan dat er geen contrast-extravasatie is |
| <input type="checkbox"/> plaatsen van een safety wire, guide wire of access sheath | <input type="checkbox"/> plaatsen van een ureter-catheter of JJ-catheter |
| <input type="checkbox"/> tijdens de steenbehandeling | <input type="checkbox"/> alleen bij (verdenking op) problemen met toegang, steenbehandeling of plaatsen ureter-catheter of JJ-catheter |
| <input type="checkbox"/> overige (geef nadere toelichting) | |

13. Hoe bepaalt U de steenvrijheid op het einde van een ingreep?

- | | |
|---|--|
| <input type="radio"/> endoscopisch en met doorlichting | <input type="radio"/> enkel met doorlichting |
| <input type="radio"/> enkel endoscopisch | <input type="radio"/> niet |
| <input type="radio"/> overige (geef nadere toelichting) | |

14. Documenteert U de per-operatieve stralingstijd en cumulatieve stralingsdosis na de ingreep?

- ja, beide
- ja, maar enkel de stralingstijd
- ja, maar enkel de cumulatieve stralingsdosis
- neen